


Comparison of Protein Assays

Uptima MicroBC Assay #UP75860A versus 1 competitor

Protein assays, all based on bicinchoninic acid method, were compared according to a standard protocol in microplate, with a same standard protein, Bovine Albumin #UP36859A.

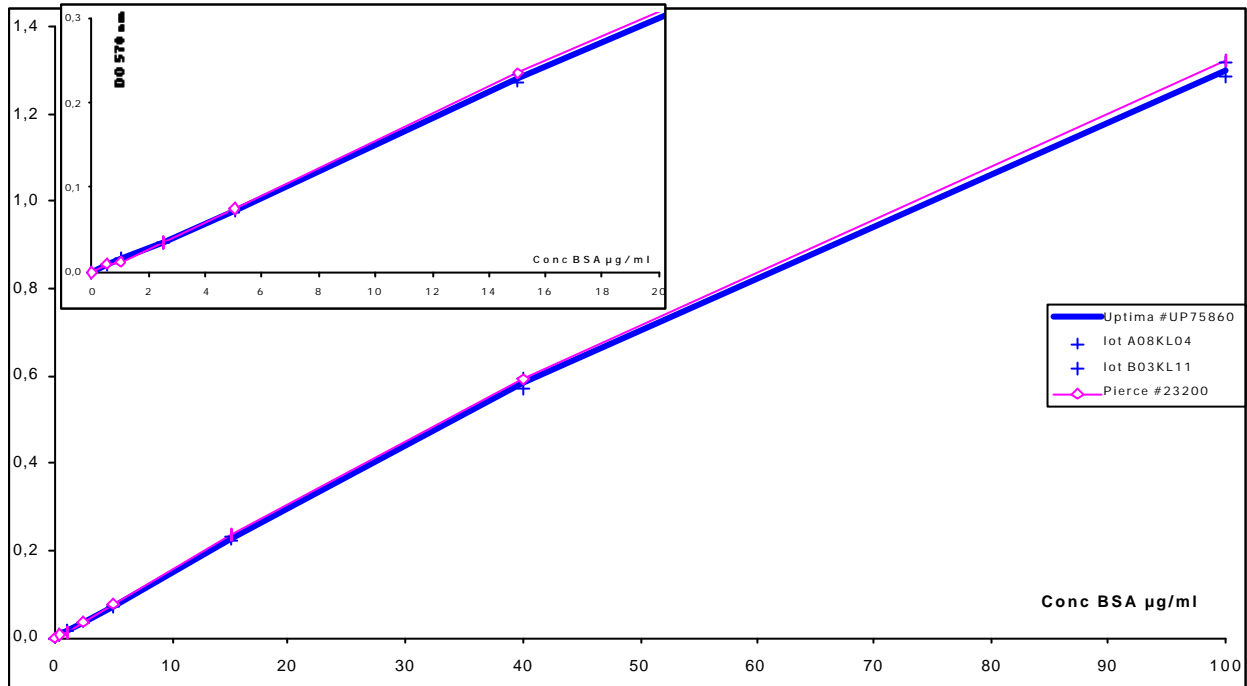

Conclusion

Uptima kit gives excellent results in sensitivity and linearity.


Remarks: Other characteristics of Uptima BC Assay are very similar or even better.

-For example, all tested substances were found compatible in the very similar extend (not shown here) as expected from the fact the assays are based on the same chemical reaction.

-Uptima offers 2 sizes of kits (1L and 50ml of final reagent)

-The packaging is more economical and convenient (albumin in screwed autostable microtubes).

DT-75860

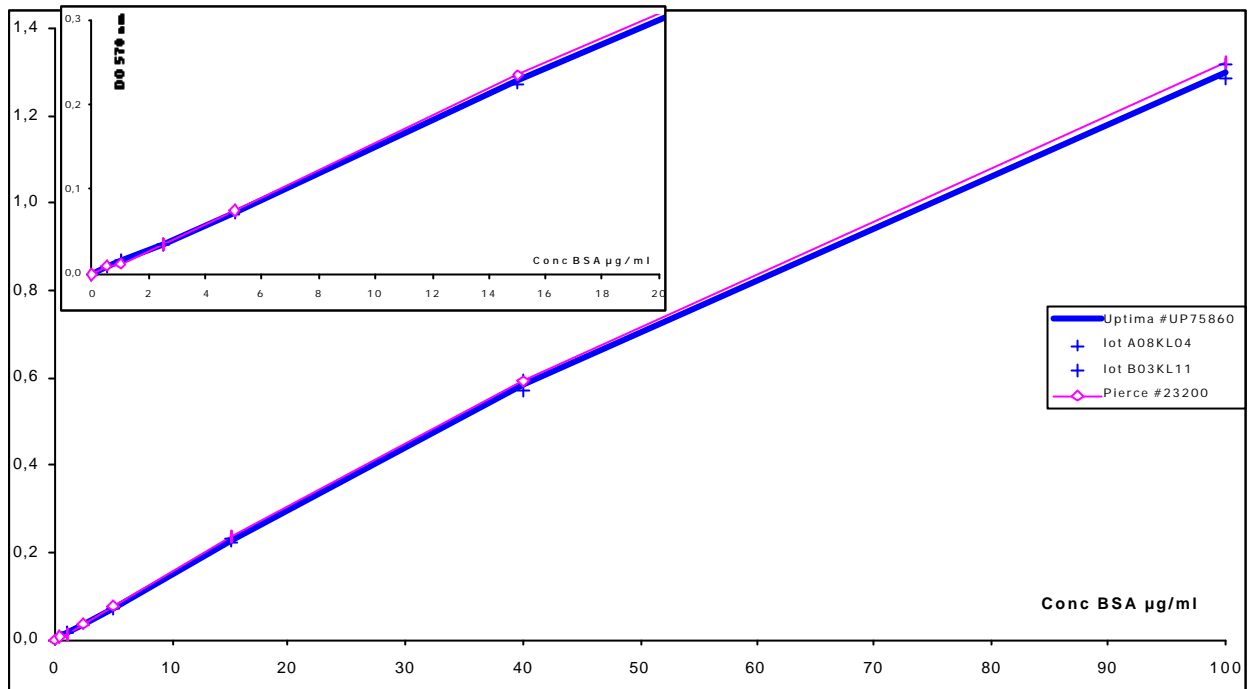

Contact your local distributor



Uptima, powered by

213 Avenue J.F. Kennedy - BP 1140
93163 Montreuil Cedex - France
Tél. 04 70 03 88 55 - Fax 04 70 03 82 86

Uptima@interchim.com